



Protocol: Identify Conditions that Solubilize Reversibly Aggregated Protein Samples


Materials:

- Aggregated protein sample (ca. 100 µL – 200 µL of total volume for each protein sample to be tested).
- An Inspection Plate with 2 x 96 OptiResc experiment wells. Two different experiments can be performed per plate or duplicate experiments per plate. An experiment requires ca. 100 µL of protein sample, duplicate experiments require 200 µL. (Up to 6 different experiments can be performed using a kit).
- OptiReagent plate.
- Multichannel pipette is recommended.

Protocol for duplicate solubilization experiments:

- Distribute 50 µL aliquots from wells of the OptiReagent plate into reservoir wells of the OptiResc Inspection Plate (all 96 wells).
- Transfer 1.0 µL of reagent from each reservoir well of the OptiResc Inspection Plate to each of the adjacent experiment wells.
- Add 1.0 µL of aggregated protein sample to experiment wells of the OptiResc Inspection Plate. Omit sample in position H1 (negative control).
- Seal OptiResc Inspection Plate with one Seal Sheet.
- Inspect small wells with a microscope, i.e. a dissecting stereo microscope and note the wells that contain precipitate (aggregated protein solution) or clear drops (dissolved protein).
If no clear drops are seen, inspect again after 1 hour or 1 day.
- Employ OptiReagent Listing (see reverse side of this brochure or www.predictive-oncology.com to identify solutions that yield clear drops.

Scale up disaggregation reaction by mixing equal volumes of aggregated protein sample with solution that was identified with the OptiResc kit.

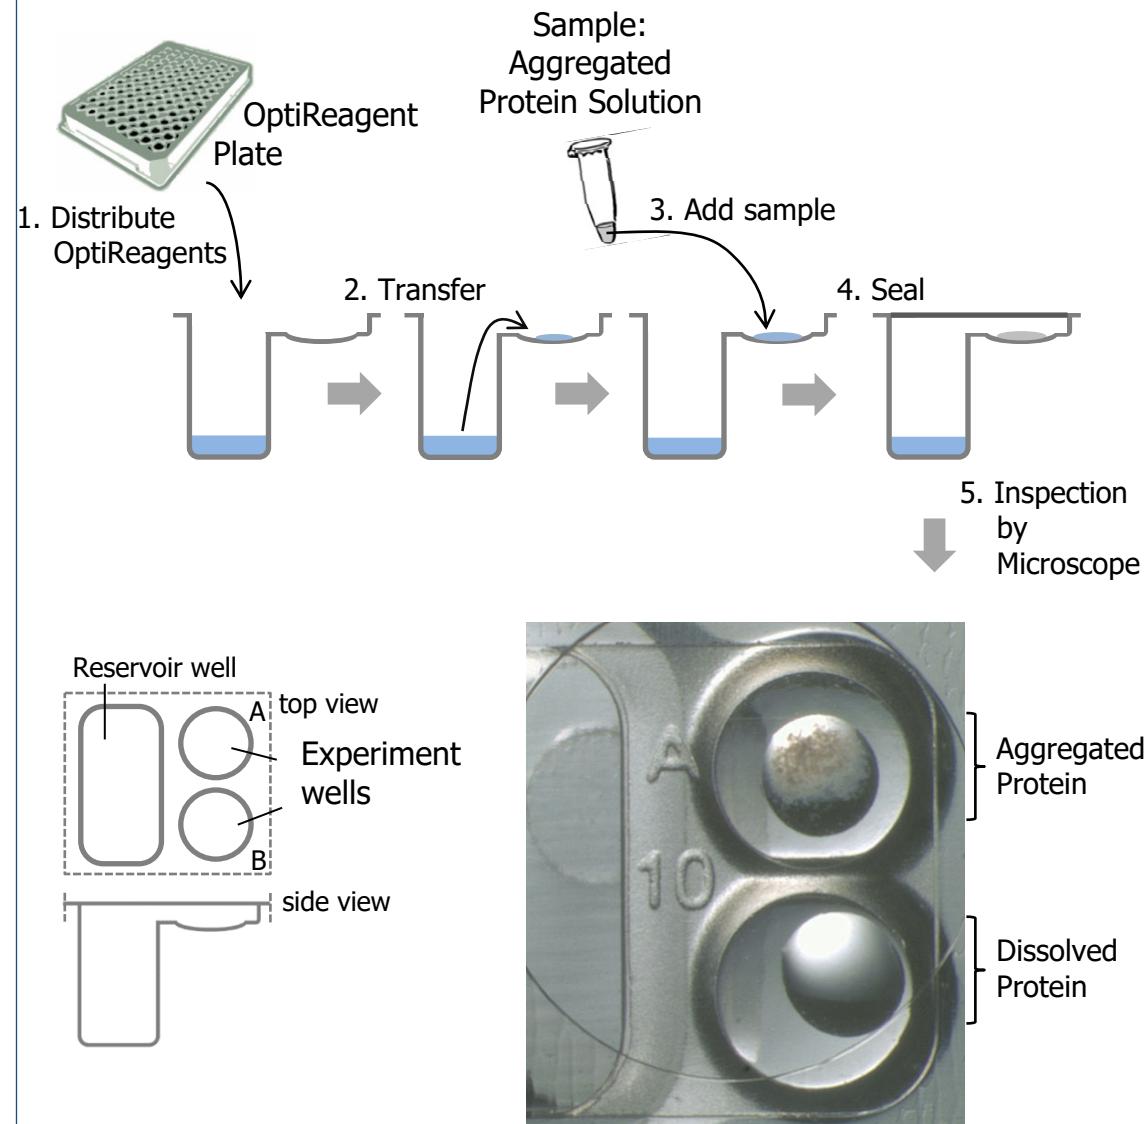

OptiResc™ Protein Aggregate Solubilization Kit

Product Information

Content:

- 1 x 96 well OptiReagent Plate
- 3 x 96 x 2 well OptiResc Inspection Plate
- 3 x 96 well Seal sheets
- Quick Start Guide and MSDS

Purpose

OptiResc Protein Aggregate Solubilization Kit

Systematic solution design and array-based deaggregation technology for:

• Solubilizing reversibly aggregated protein samples

For updated instructions and additional information please refer to www.predictive-oncology.com.

One OptiResc kit contains all consumable materials to search solution conditions for up to six (6) different, reversibly aggregated protein samples.

Order Information

Order Cat #: SOL-Resc

OptiResc Protein Aggregate Solubilization Kit

Price: \$399 USD (3 pack for \$999 USD)

Predictive Oncology

200 Riverhills Business Park www.predictive-oncology.com
Ste. 250 orders@predictive-oncology.com
Birmingham, AL 35242 USA

Reagent Listing

Well # Row Col	Buffer [#]	Additive	
		NAME	Conc unit
1 A 1	Glycine	100 mM	3.0
2 A 2	Citric Acid	100 mM	3.2
3 A 3	PIPPS	100 mM	3.7
4 A 4	Citric Acid	100 mM	4.0
5 A 5	Sodium Acetate	100 mM	4.5
6 A 6	Na/K Phosphate	100 mM	5.0
7 A 7	Sodium Citrate	100 mM	5.5
8 A 8	Na/K Phosphate	100 mM	6.0
9 A 9	Bis-Tris	100 mM	6.0
10 A 10	MES	100 mM	6.2
11 A 11	ADA	100 mM	6.5
12 A 12	Bis-Tris Propane	100 mM	6.5
13 B 1	Ammonium Acetate	100 mM	7.0
14 B 2	MOPS	100 mM	7.0
15 B 3	Na/K Phosphate	100 mM	7.0
16 B 4	HEPES	100 mM	7.5
17 B 5	Tris	100 mM	7.5
18 B 6	EPPS	100 mM	8.0
19 B 7	Imidazole	100 mM	8.0
20 B 8	Bicine	100 mM	8.5
21 B 9	Tris	100 mM	8.5
22 B 10	CHES	100 mM	9.0
23 B 11	CHES	100 mM	9.5
24 B 12	CAPS	100 mM	10.0
25 C 1	Glycine	50 mM	3.0
26 C 2	Sodium Acetate	50 mM	4.5
27 C 3	Bis-Tris	50 mM	6.0
28 C 4	MOPS	50 mM	7.0
29 C 5	Imidazole	50 mM	8.0
30 C 6	CHES	50 mM	9.5
31 C 7	Citric Acid	50 mM	3.2
32 C 8	Na/K Phosphate	50 mM	5.0
33 C 9	ADA	50 mM	6.5
34 C 10	HEPES	50 mM	7.5
35 C 11	Tris	50 mM	8.5
36 C 12	CAPS	50 mM	10.0
37 D 1	Glycine	50 mM	3.0
38 D 2	Sodium Acetate	50 mM	4.5
39 D 3	Bis-Tris	50 mM	6.0
40 D 4	MOPS	50 mM	7.0
41 D 5	Imidazole	50 mM	8.0
42 D 6	CHES	50 mM	9.5
43 D 7	Citric Acid	50 mM	3.2
44 D 8	Na/K Phosphate	50 mM	5.0
45 D 9	ADA	50 mM	6.5
46 D 10	HEPES	50 mM	7.5
47 D 11	Tris	50 mM	8.5
48 D 12	CAPS	50 mM	10.0
49 E 1	Trehalose	500 mM	
50 E 2	Trehalose	500 mM	
51 E 3	Trehalose	500 mM	
52 E 4	Trehalose	500 mM	
53 E 5	Trehalose	500 mM	
54 E 6	Trehalose	500 mM	
55 E 7	Trehalose	500 mM	
56 E 8	Trehalose	500 mM	
57 E 9	Trehalose	500 mM	
58 E 10	Trehalose	500 mM	
59 E 11	Trehalose	500 mM	
60 E 12	Trehalose	500 mM	
61 F 1	Trehalose	500 mM	
62 F 2	Trehalose	500 mM	
63 F 3	Trehalose	500 mM	
64 F 4	Trehalose	500 mM	
65 F 5	Trehalose	500 mM	
66 F 6	Trehalose	500 mM	
67 F 7	Trehalose	500 mM	
68 F 8	Trehalose	500 mM	
69 F 9	Trehalose	500 mM	
70 F 10	Trehalose	500 mM	
71 F 11	Trehalose	500 mM	
72 F 12	Trehalose	500 mM	
73 G 1	Trehalose	500 mM	
74 G 2	Trehalose	500 mM	
75 G 3	Trehalose	500 mM	
76 G 4	Trehalose	500 mM	
77 G 5	Trehalose	500 mM	
78 G 6	Trehalose	500 mM	
79 G 7	Trehalose	500 mM	
80 G 8	Trehalose	500 mM	
81 G 9	Trehalose	500 mM	
82 G 10	Trehalose	500 mM	
83 G 11	Trehalose	500 mM	
84 G 12	Trehalose	500 mM	
85 H 1	Trehalose	500 mM	
86 H 2	Trehalose	500 mM	
87 H 3	Trehalose	500 mM	
88 H 4	Trehalose	500 mM	
89 H 5	Trehalose	500 mM	
90 H 6	Trehalose	500 mM	
91 H 7	Trehalose	500 mM	
92 H 8	Trehalose	500 mM	
93 H 9	Trehalose	500 mM	
94 H 10	Trehalose	500 mM	
95 H 11	Trehalose	500 mM	
96 H 12	Trehalose	500 mM	

Well # Row Col	Buffer [#]	Additive	
		NAME	Conc unit
49 E 1	Glycine	50 mM	3.0
50 E 2	Sodium Acetate	50 mM	4.5
51 E 3	Bis-Tris	50 mM	6.0
52 E 4	MOPS	50 mM	7.0
53 E 5	Imidazole	50 mM	8.0
54 E 6	CHES	50 mM	9.5
55 E 7	Citric Acid	50 mM	3.2
56 E 8	Na/K Phosphate	50 mM	5.0
57 E 9	ADA	50 mM	6.5
58 E 10	HEPES	50 mM	7.5
59 E 11	Tris	50 mM	8.5
60 E 12	CAPS	50 mM	10.0
61 F 1	Glycine	50 mM	3.0
62 F 2	Sodium Acetate	50 mM	4.5
63 F 3	Bis-Tris	50 mM	6.0
64 F 4	MOPS	50 mM	7.0
65 F 5	Imidazole	50 mM	8.0
66 F 6	CHES	50 mM	9.5
67 F 7	Citric Acid	50 mM	3.2
68 F 8	Na/K Phosphate	50 mM	5.0
69 F 9	ADA	50 mM	6.5
70 F 10	HEPES	50 mM	7.5
71 F 11	Tris	50 mM	8.5
72 F 12	CAPS	50 mM	10.0
73 G 1	Glycine	50 mM	3.0
74 G 2	Sodium Acetate	50 mM	4.5
75 G 3	Bis-Tris	50 mM	6.0
76 G 4	MOPS	50 mM	7.0
77 G 5	Imidazole	50 mM	8.0
78 G 6	CHES	50 mM	9.5
79 G 7	Citric Acid	50 mM	3.2
80 G 8	Na/K Phosphate	50 mM	5.0
81 G 9	ADA	50 mM	6.5
82 G 10	HEPES	50 mM	7.5
83 G 11	Tris	50 mM	8.5
84 G 12	CAPS	50 mM	10.0
85 H 1	Trehalose	500 mM	
86 H 2	Trehalose	500 mM	
87 H 3	Trehalose	500 mM	
88 H 4	Trehalose	500 mM	
89 H 5	Trehalose	500 mM	
90 H 6	Trehalose	500 mM	
91 H 7	Trehalose	500 mM	
92 H 8	Trehalose	500 mM	
93 H 9	Trehalose	500 mM	
94 H 10	Trehalose	500 mM	
95 H 11	Trehalose	500 mM	
96 H 12	Trehalose	500 mM	
97 H 1	AmSulfate	3 M	
98 H 2	Acetonitrile	80 % (v/v)	
99 H 3	NaCl	50 mM	
100 H 4	DTT	1 mM	
101 H 5	DTT	5 mM	
102 H 6	DTT	15 mM	
103 H 7	BME	2.5 mM	
104 H 8	BME	10 mM	
105 H 9	BME	20 mM	

TMAO, Trimethylamine N-Oxide; PIPPS, Piperazine-N, n'-Bis (3-Propanesulfonic Acid); MES, 2-(N-morpholino) ethanesulfonic acid; MOPS, 3-(N-morpholino) propanesulfonic acid; HEPES, 4-(2-hydroxyethyl)-1-piperazineethanesulfonic acid; Arg/Glu*: 50mM of each Arginine and Glutamate; DDT, DL-Dithiothreitol; BME, 2-Mercaptoethanol; Betaine, Trimethyl-Glycine; CAPS, N-cyclohexyl-3-amino-propanesulfonic acid; ADA, N-(2-Acetamido)iminoacetic Acid; Tris, tris(hydroxymethyl)aminomethane; CHES, 2-(N-Cyclohexylamino)ethane Sulfonic Acid; EPPS, N-(2-hydroxyethyl)piperazine-N-(3-propanesulfonic acid).

* pH values for buffers used only; * each amino acid is 50 mM